


12. Standard sugars

Data No. LA067-0000

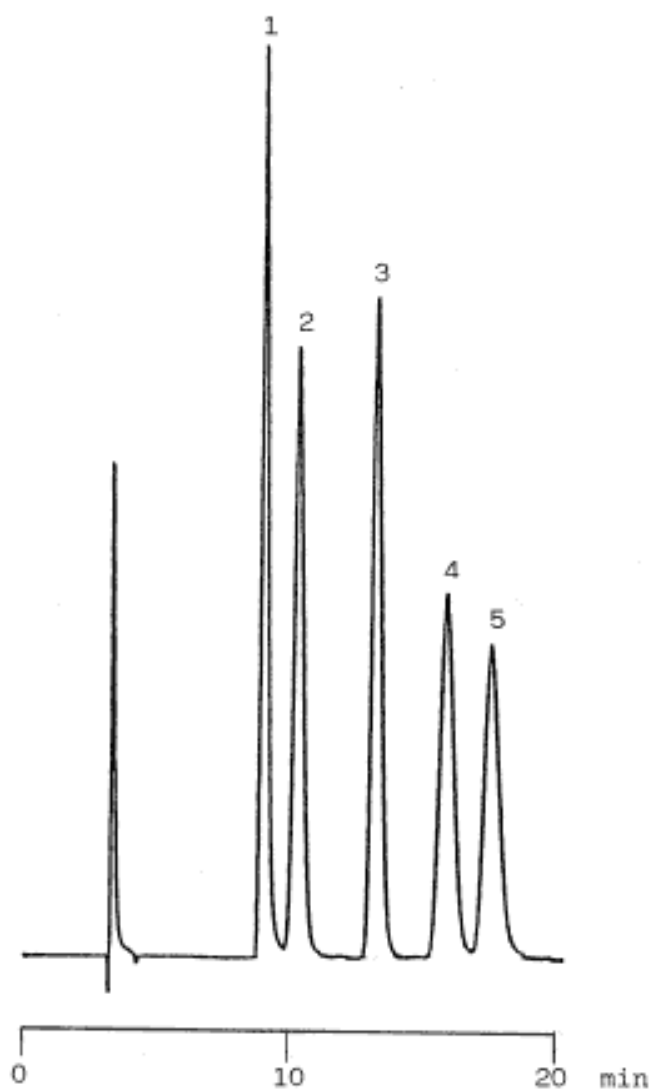

Column : Unisil Q NH2
5 μ m
250 $\times$ 4.6 mm I.D.

Column Cat. No. : 5020-03402

Eluent : CH₃CN/H₂O = 70/30

Flow rate : 1.0 mL/min.

Col. Temp. : 25°C

Detection : RI

Injection Vol. :

Sample : Sugars

Solutes : 1. Fructose
2. Glucose
3. Sucrose
4. Maltose
5. Lactose