
31. Analysis of Aflatoxin

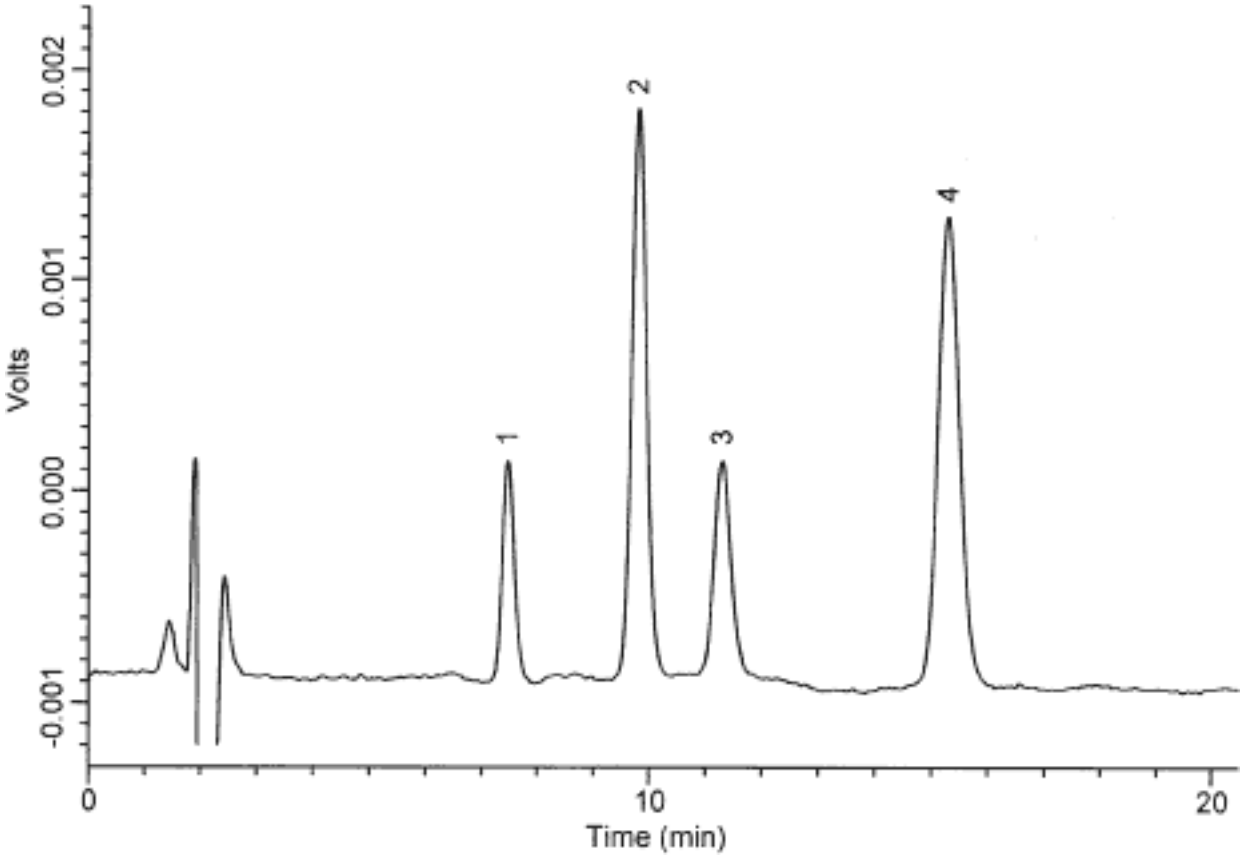

Column	:Inertsil C8-3
	150 × 4.6 mm I.D.
Column Cat. No.	:
Eluent	:CH_3OH/H_2O = 40/60
Flow rate	:1.0 mL/min.
Col. Temp.	:40°C
Detection	:UV 365 nm
Injection Vol.	:100 µL
Sample	:Aflatoxins

Solutes : 1. Aflatoxin G2 (0.06 µg/mL)
2. Aflatoxin G1 (0.20 µg/mL)
3. Aflatoxin B2 (0.06 µg/mL)
4. Aflatoxin B1 (0.20 µg/mL)