


Analysis of Flurbiprofen

Data No. LA168-0000

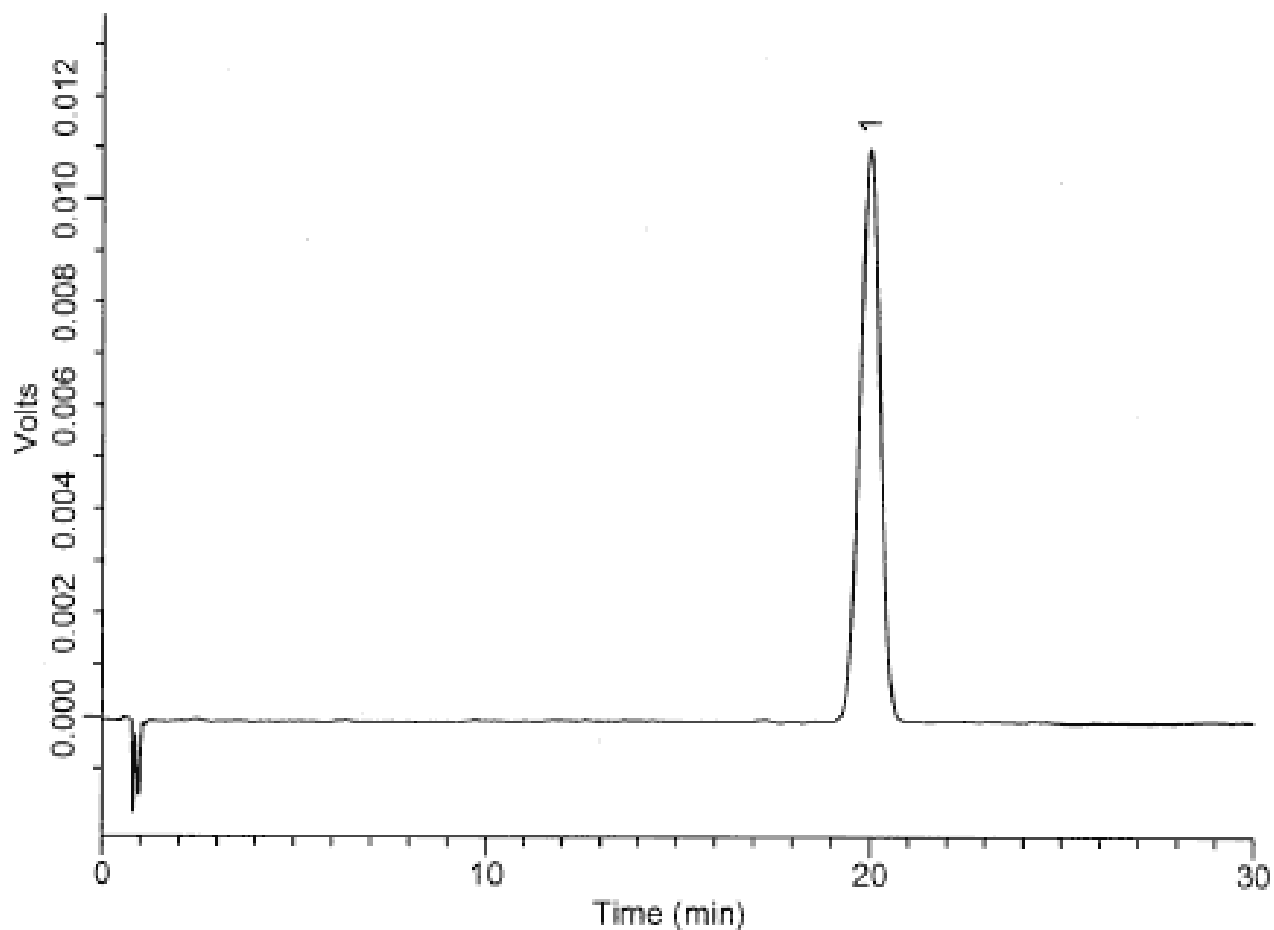

Column : Inertsil ODS-3V
150 × 4.6mmI.D. Solutes : 1. Flurbiprofen(20µg/mL)

Column Cat. No. :

Eluent : CH₃CN/H₂O/CH₃COOH=7/12/1

Flow rate : 1.9 mL/min.

Col. Temp. : 30°C

Detection : UV 254 nm

Injection Vol. : 20µL

Sample : Flurbiprofen(20µg/mL)