

Analysis of Biotin

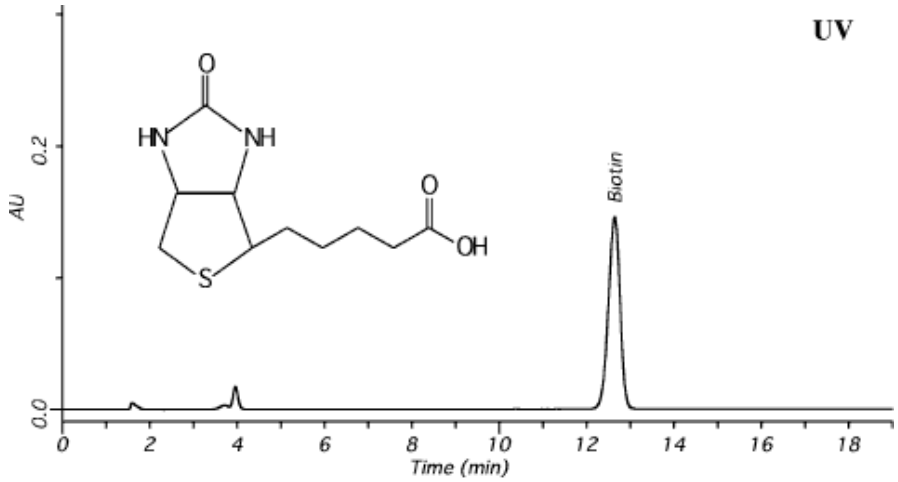

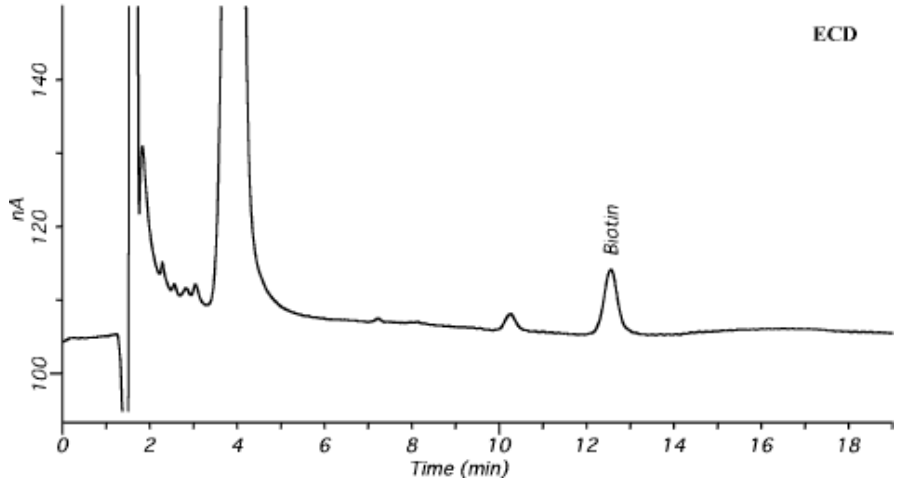

Column	:Inertsil ODS-3
	5µm
	150 × 4.6mmI.D.
Column Cat. No.	:
Eluent	:Acetonitrile / 50 mM KH2PO4 (pH = 4.0 adjusted by H3PO4) = 10 / 90
Flow rate	:1.0mL/min
Col. Temp.	:40ºC
Detection	:UV 210 nm
	ECD 1000 mV vs. Ag / AgCl (Diamond)
Injection Vol.	:10µL
Sample	:1 mg / ml Biotin in 20 mM K2HPO4
Solutes	:Biotin