


Analysis of Endocrine Disrupters

Data No. LA340-0000

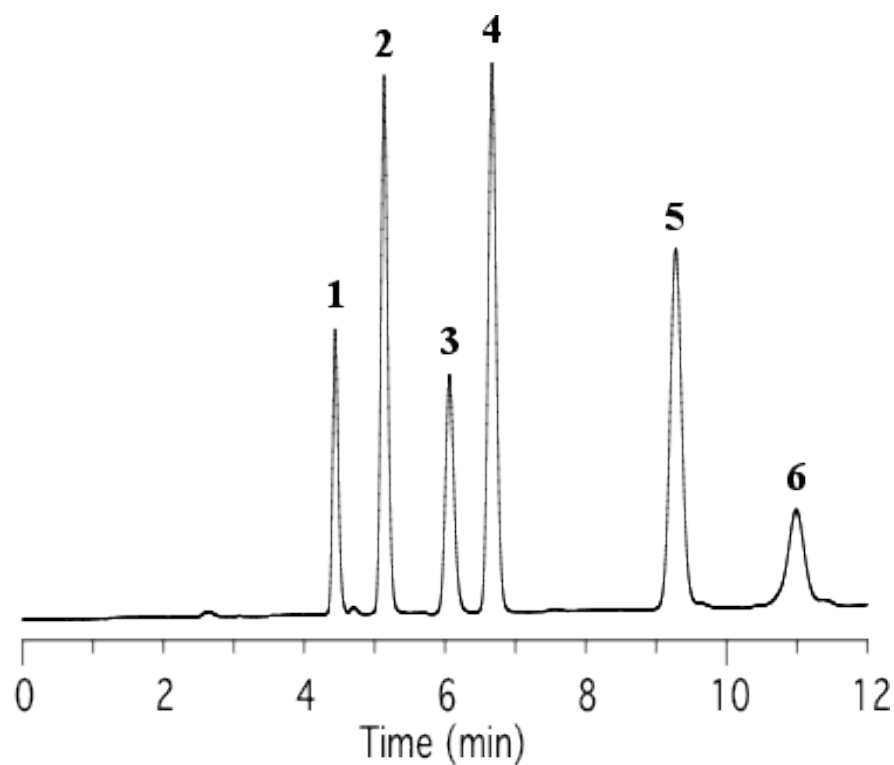

Column : Inertsil CN-3
5 μ m
250 x 4.6 mm I.D.

Column Cat. No. :

Eluent : A) CH₃CN
B) 20 mM Phosphate buffer (pH 3.0)
A/B = 45/55, v/v

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 280 nm

Injection Vol. : 3 μ L

Sample :

Solutes : 1. Phenol (0.06 mg/mL)
2. Diethyl phthalate (0.12 mg/mL)
3. Bisphenol A (0.02 mg/mL)
4. 2,4-Dichlorophenol (0.06 mg/mL)
5. 4-Octylphenol (0.12 mg/mL)
6. 4-Nonylphenol (0.12 mg/mL)