


Purification of C60 Buckminsterfullerene

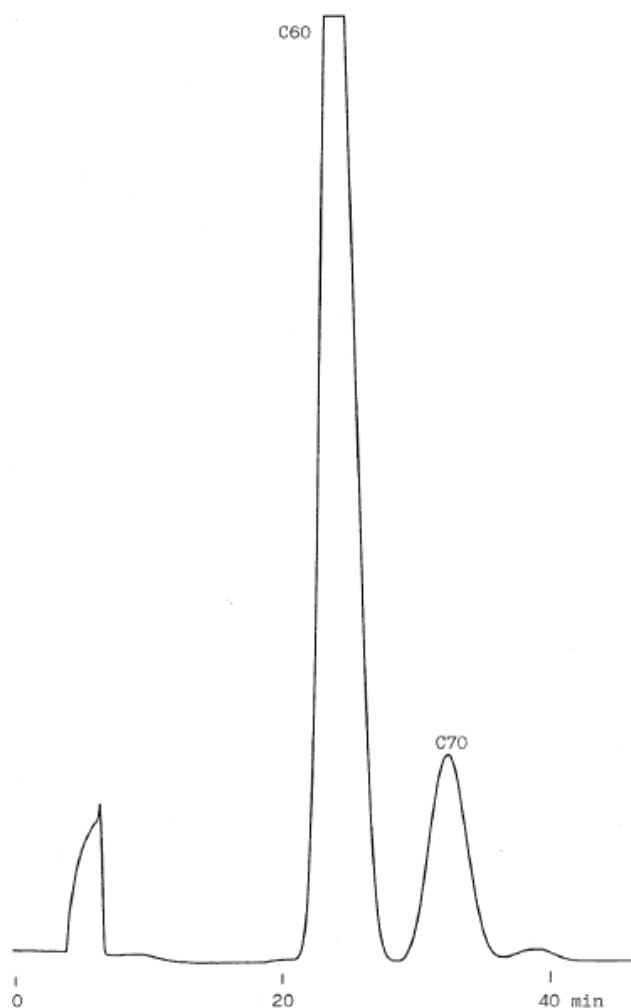

Column :ECONOPREP ODS
40 μ m
500 $\times$ 100 mm I.D.

Solutes : 1. C60 (0.01 % in Eluent)
2. C70 (0.01 % in Eluent)

Column Cat. No. :5020-36085

Eluent :Toluene/CH₃CN = 60/40

Flow rate :280 mL/min.

Col. Temp. :

Detection :UV 350 nm

Injection Vol. :1000 μ L

Sample :Crude C60, C70