


InertSearch™ for LC

Inertsil® Applications

Analysis of purine derivatives by LC/MS/MS

Data No. LA621-0696

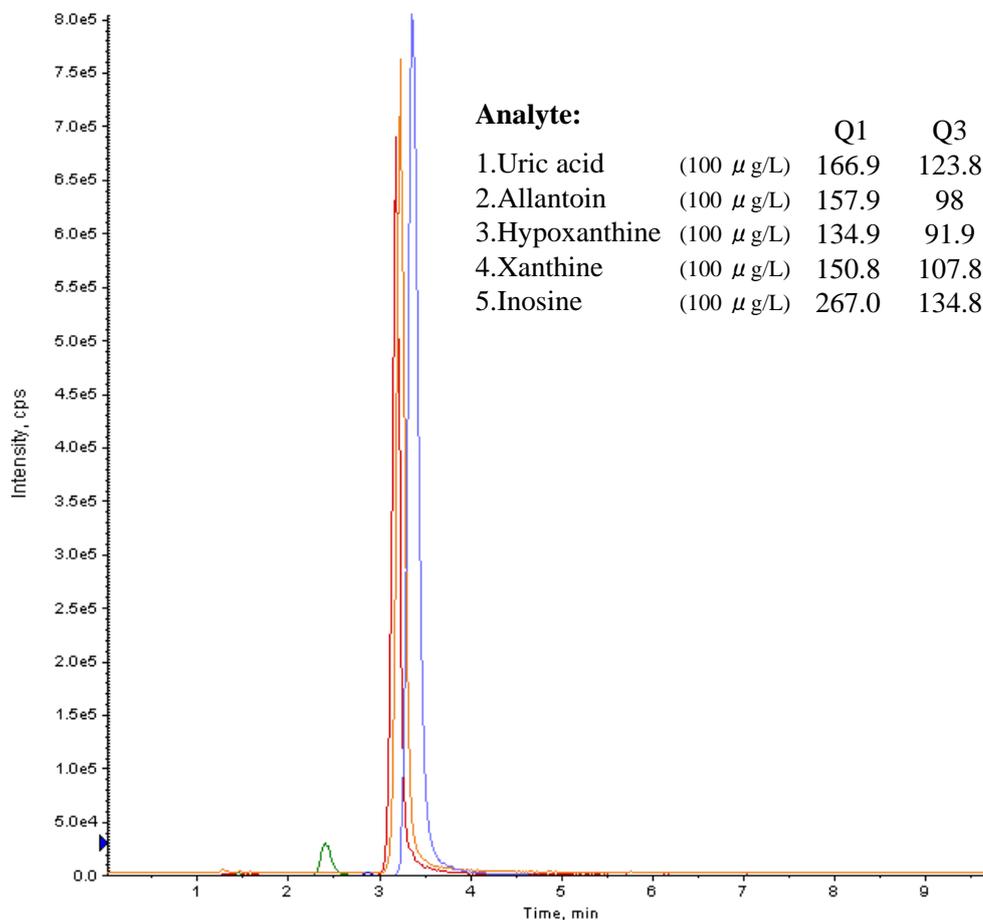

Conditions

System : LC800 HPLC system
4000 Q TRAP®

Column : Inertsil HILIC (5 µm, 150 x 2.1 mm I.D.)

Column Cat. No. : 5020-07705

Eluent : A) CH₃CN
B) 2 mM Ammonium acetate
A/B = 90/10, v/v

Flow Rate : 0.3 mL/min

Col. Temp. : 40 °C

Detection : LC/MS/MS (4000 Q TRAP®: ESI, Negative, MRM)

CUR	CAD	IS	TEM	GS1	GS2
10	8	-4500	700	60	30

Injection Vol. : 10 µL

Sample : Purine derivatives

InertSearch™ for LC

Inertsil® Applications

Analysis of purine derivatives by LC/MS/MS

Data No. LA621-0696

