


## Analysis of Nucleotides (Inertsil ODS-4)

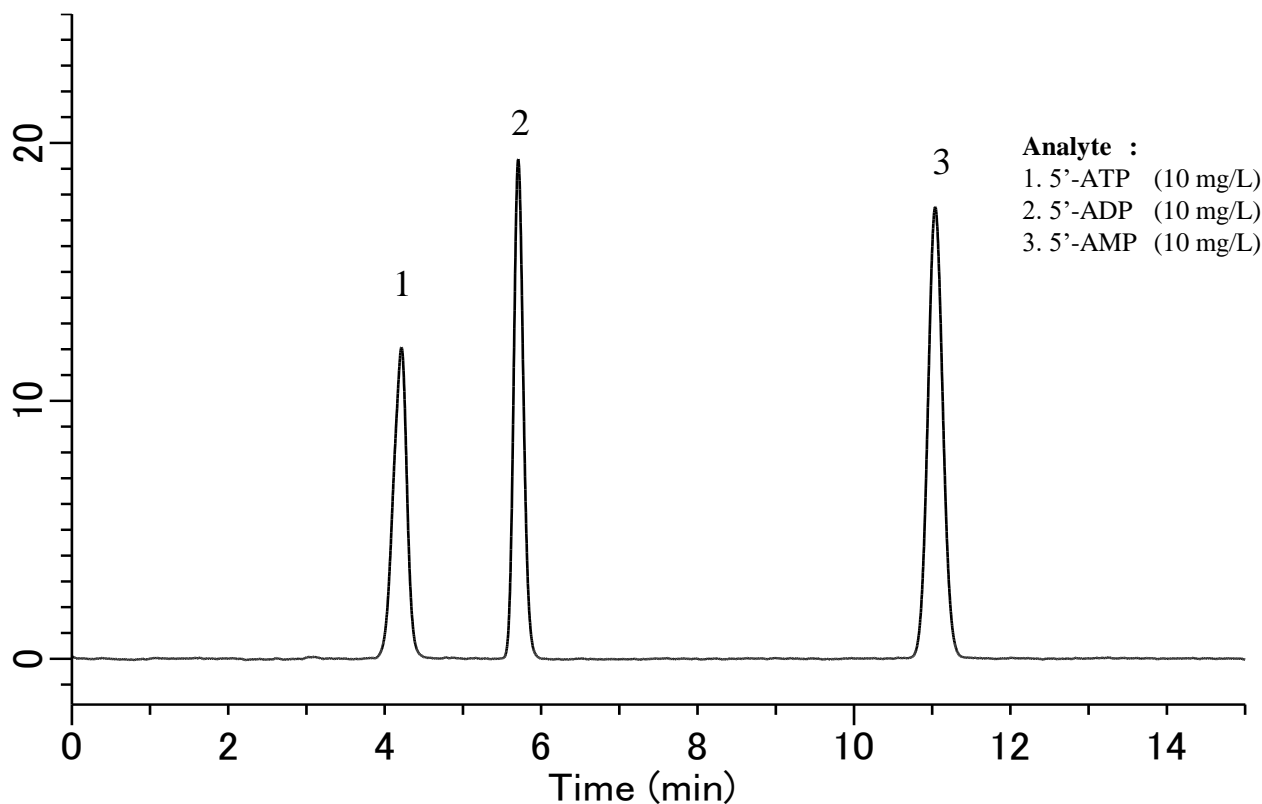

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil ODS-4 (5  $\mu$ m, 250 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-03946  
**Eluent** : 10 mM Na<sub>2</sub>HPO<sub>4</sub> (pH 6.0, H<sub>3</sub>PO<sub>4</sub>)  
**Flow Rate** : 1.0 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 260 nm (GL-7450 UV Detector)  
**Injection Vol.** : 10  $\mu$ L  
**Sample** : Nucleotides