


Analysis of Proteins

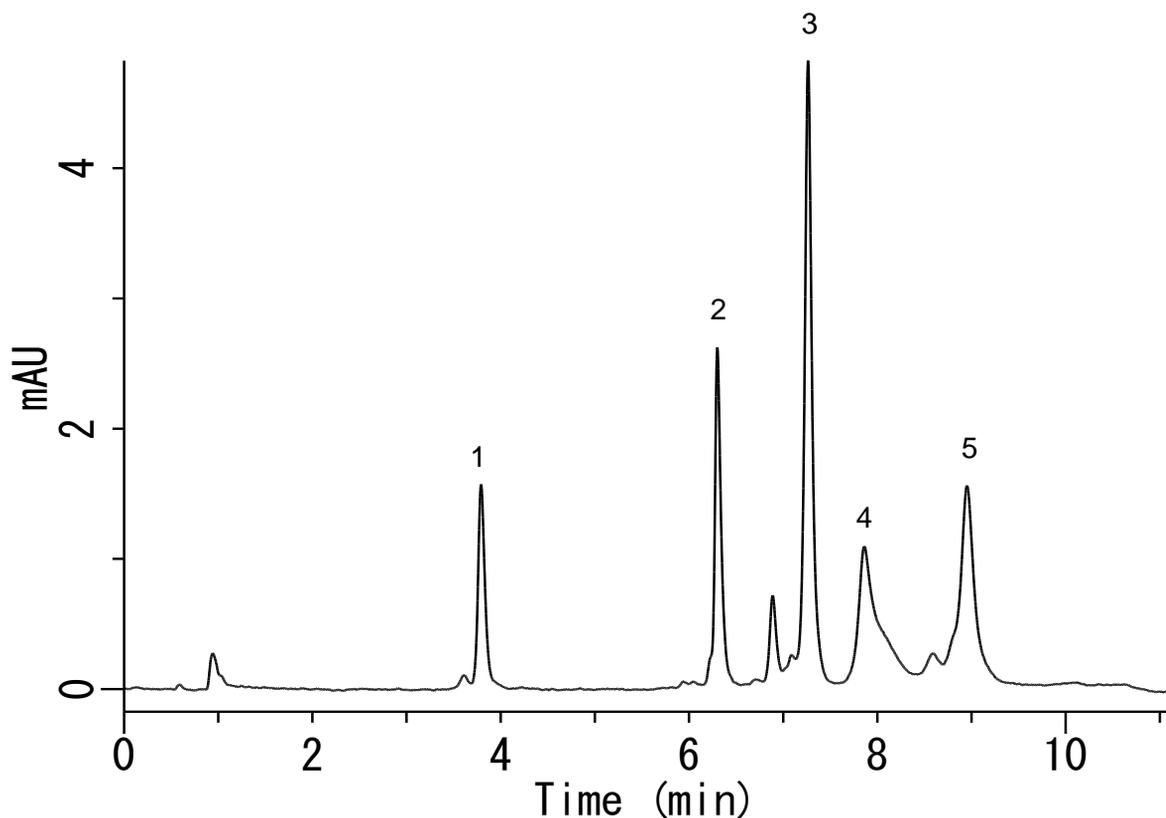

Conditions

System : GL-7400 HPLC System
Column : MonoClad C18-HS (150 x 3.0 mm I.D.)
Column Cat. No. : 5020-10803
Eluent : A) 0.1 % TFA in H₂O
 : B) 0.1 % TFA in CH₃CN
 : A/B = 75/25 – 10 min - 50/50, v/v
Flow Rate : 1 mL/min
Col. Temp. : 40 °C
Detection : UV 280 nm (GL-7450 UV Detector)
Injection Vol. : 1 µL

Analyte

1. Ribonuclease A
2. Cytochrome C
3. Lysozyme
4. Transferrin
5. Conalbumin