


## Analysis of Ergosterol(Inertsil ODS-4)

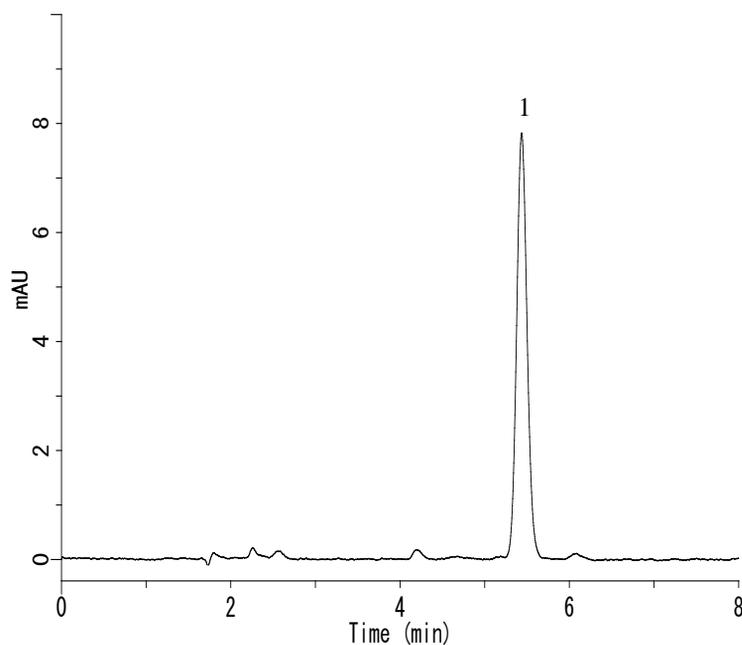

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil ODS-4 (5  $\mu$ m, 150 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-03945  
**Eluent** : CH<sub>3</sub>OH  
**Flow Rate** : 1.0 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 290 nm (GL-7450 UV Detector)  
**Injection Vol.** : 10  $\mu$ L  
**Sample** : Standard

### Analyte

1. Ergosterol (10 mg/L)