


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Pre-column Derivatized Amino Acids

Data No. LB088-0812

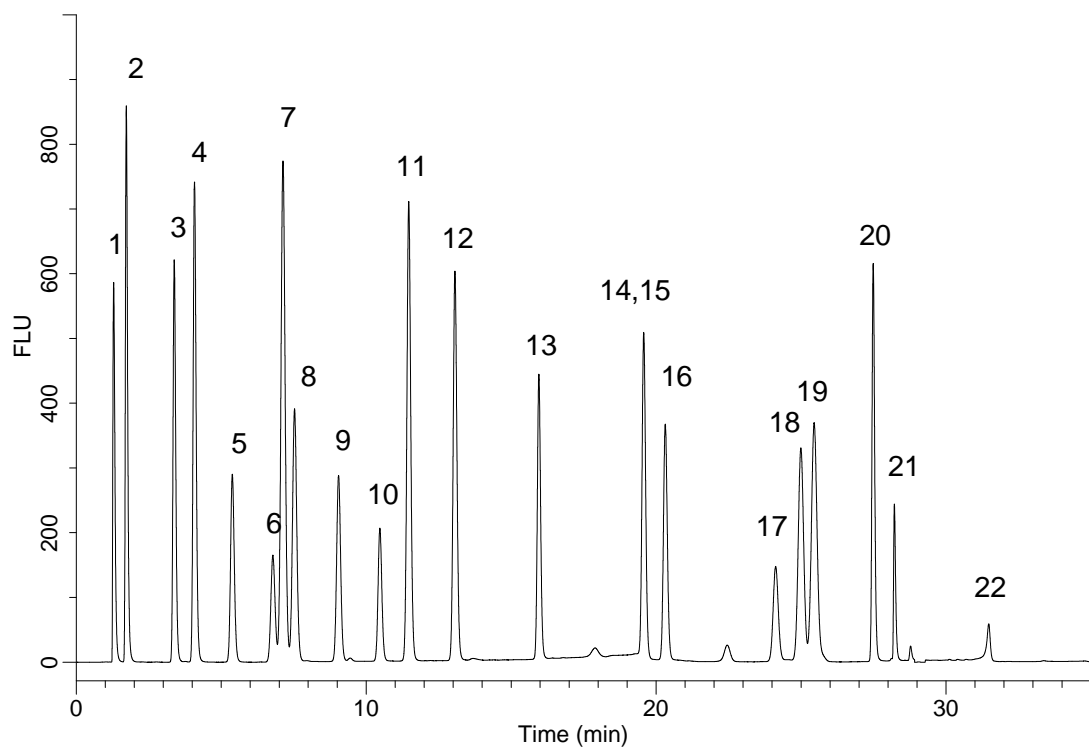

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil ODS-4  
(3  $\mu$  m, 150 x 3.0 mm I.D.)  
**Column Cat. No.** : 5020-04025  
**Eluent** : A) CH<sub>3</sub>CN/CH<sub>3</sub>OH/H<sub>2</sub>O = 45/40/15, v/v/v  
B) 20 mM KH<sub>2</sub>PO<sub>4</sub> (pH 6.9, H<sub>3</sub>PO<sub>4</sub>)

Time(min)	A (%)	B (%)
0	11	89
3	11	89
12	22	78
14	28	72
23	30	70
27	65	35
34	75	25
35	100	0

**Flow Rate** : 0.7 mL/min  
**Col. Temp.** : 35 °C  
**Detection** : FL Ex 350 nm Em 450 nm (0-29 min)  
Ex 266 nm Em 305 nm (29-35 min)  
(GL-7453 FL Detector)

**Injection Vol.** : 1  $\mu$  L  
**Sample** : Derivatized Amino Acids

### Analyte:

1. OPA-Aspartic Acid
2. OPA-Glutamic Acid
3. OPA-Asparagine
4. OPA-Serine
5. OPA-Glutamine
6. OPA-Histidine
7. OPA-Glycine
8. OPA-Threonine
9. OPA-Citrulline
10. OPA-Arginine
11. OPA-Alanine
12. OPA-GABA(4-aminobutanoic acid)
13. OPA-Tyrosine
14. OPA-Cys-Cys
15. OPA-Valine
16. OPA-Methionine
17. OPA-Tryptophan
18. OPA-Phenylalanine
19. OPA-Isoleucine
20. OPA-Leucine
21. OPA-Lysine
22. Fmoc-Proline  
(each 10  $\mu$  g/mL)