


Analysis of Urea

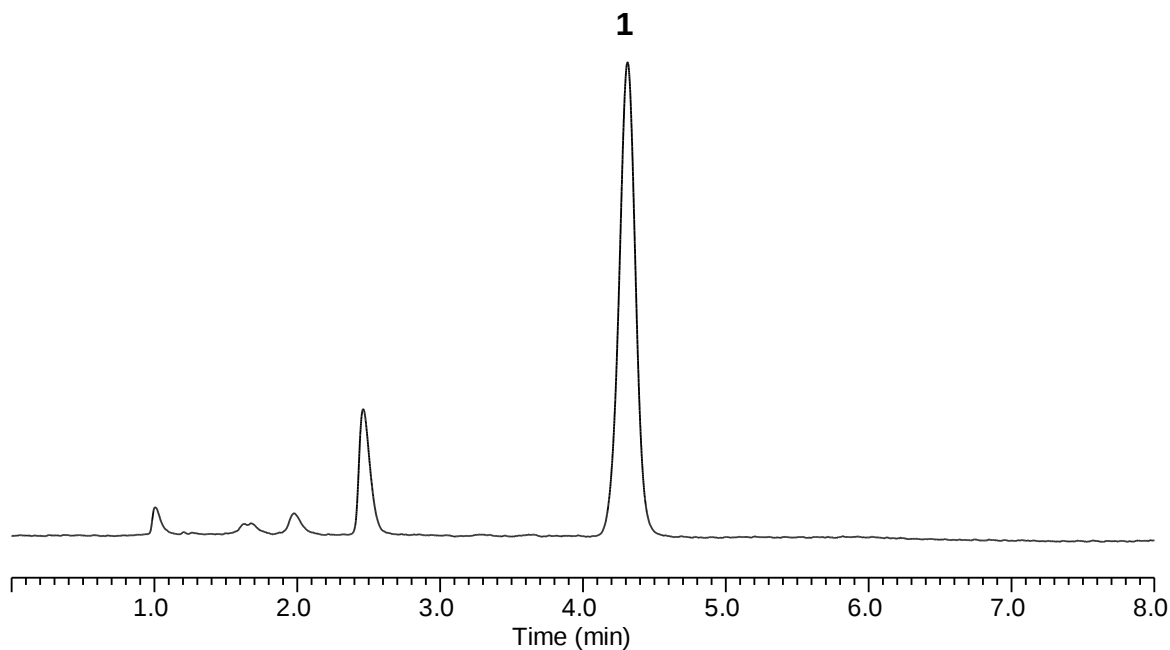

Conditions

System : LC800 HPLC System
Column : Inertsil Amide (5 μ m, 150 x 3.0 mm I.D.)
Column Cat. No. : 5020-07815
Eluent : A) CH₃CN
 : B) H₂O
 : A/B = 85/15, v/v
Flow Rate : 0.4 mL/min.
Col. Temp. : 40 °C
Detection : UV 200 nm
Injection Vol. : 5.0 μ L

Analyte

1. Urea 200 mg/L