

Catecholamines play an important role as neurotransmitter and adrenal gland hormones in the human body. Concentration of three major catecholamines (norepinephrine, epinephrine, and dopamine) in urine are significant in diagnosis and treatment of several diseases.


In this note, a determination method for urinary catecholamines using HPLC-ECD (Electrochemical detector) and MonoSpin PBA, which is a spin column

for sample pretreatment, is described. The advantage of this method is not only its simplicity but also high sensitivity and selectivity. Furthermore, this method is quite easy-to-use because cleaning of conductive diamond electrode used as the working electrode can be performed routinely without removing it from the flow cell. Manual polishing of the working electrode is not necessary at all.


(C.Aoyama)

A Chromatogram Obtained from Standard Solution

To keep the working electrode clean, high oxidation potential (+ 4000 mV) was applied between 15 min and 16 min after every sample injection. This convenient automated cleaning can be carried out owing to the extreme stability of the boron-doped diamond electrode.

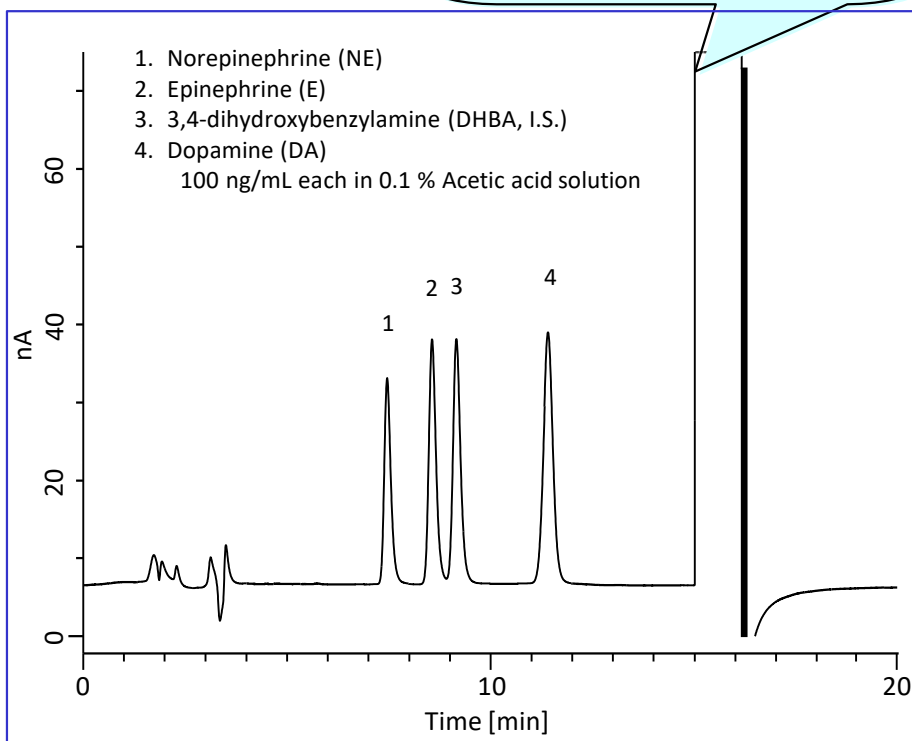

Calibration curves for three catecholamines

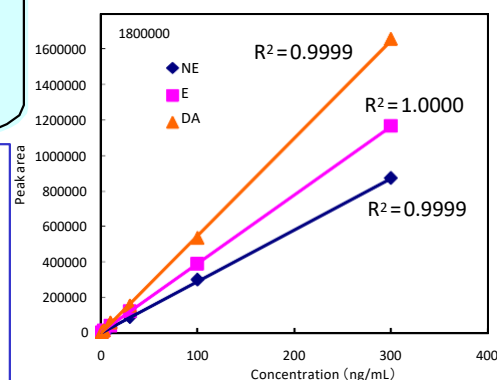


HPLC Conditions


Column : Inertsil ODS-4
(5 μ m, 250 \times 3.0 mm I.D.)
Eluent : A) Acetate-citrate buffer*
B) CH₃CN
A/B = 100/16, v/v (Premix)
Flow rate : 0.5 mL/min
Col. Temp. : 35 $^{\circ}$ C
Detection : ECD 800 mV vs. Ag/AgCl
(ED703, Diamond)
Inj. Vol. : 20 μ L

* Acetate-citrate buffer :
To 500 mL of water, 0.82 g of sodium acetate (anhydrous), 2.10 g of citric acid (monohydrate), and 0.5 g of sodium 1-octanesulfonate was dissolved.


Chemical Structure

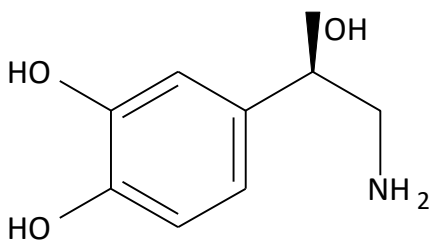


Norepinephrine (NE)
or noradrenaline

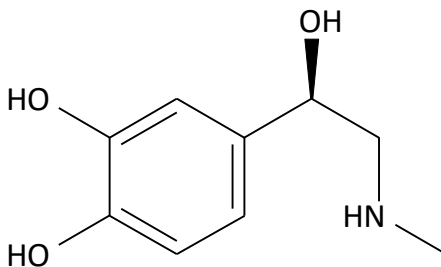

Epinephrine (E)
or adrenaline

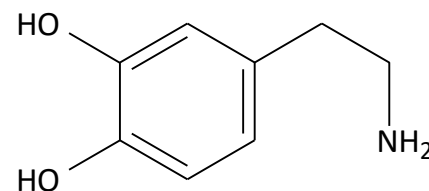


Dopamine (DA)

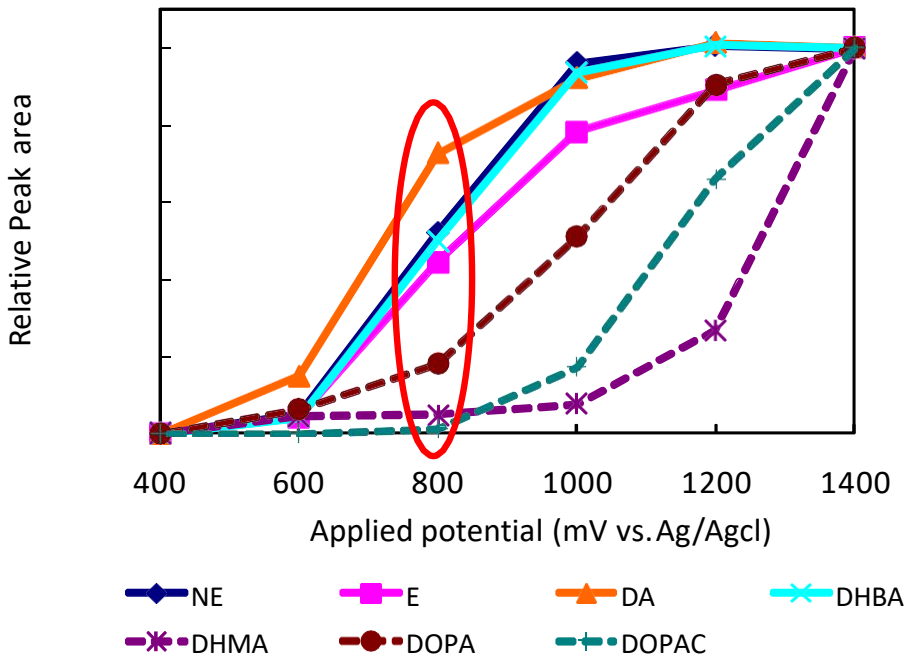


Setting the potential at + 800 mV enables us to diminish peaks of other compounds in sample solution and to detect catecholamines with high selectivity.

A chromatogram at + 800 mV

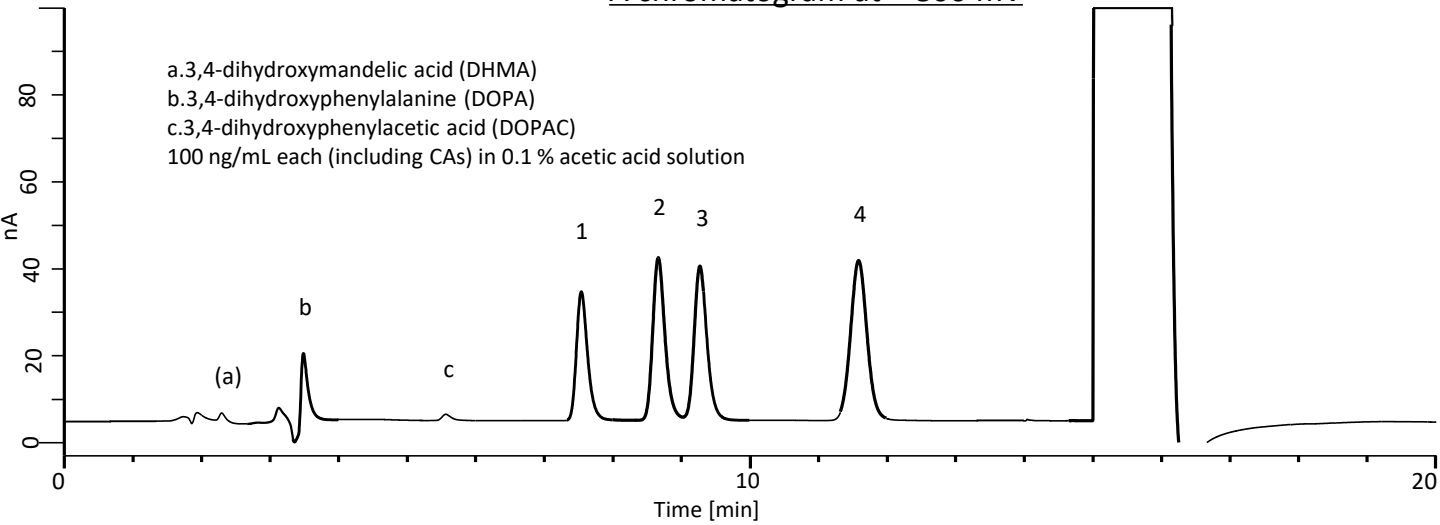



A chromatogram at + 1400 mV

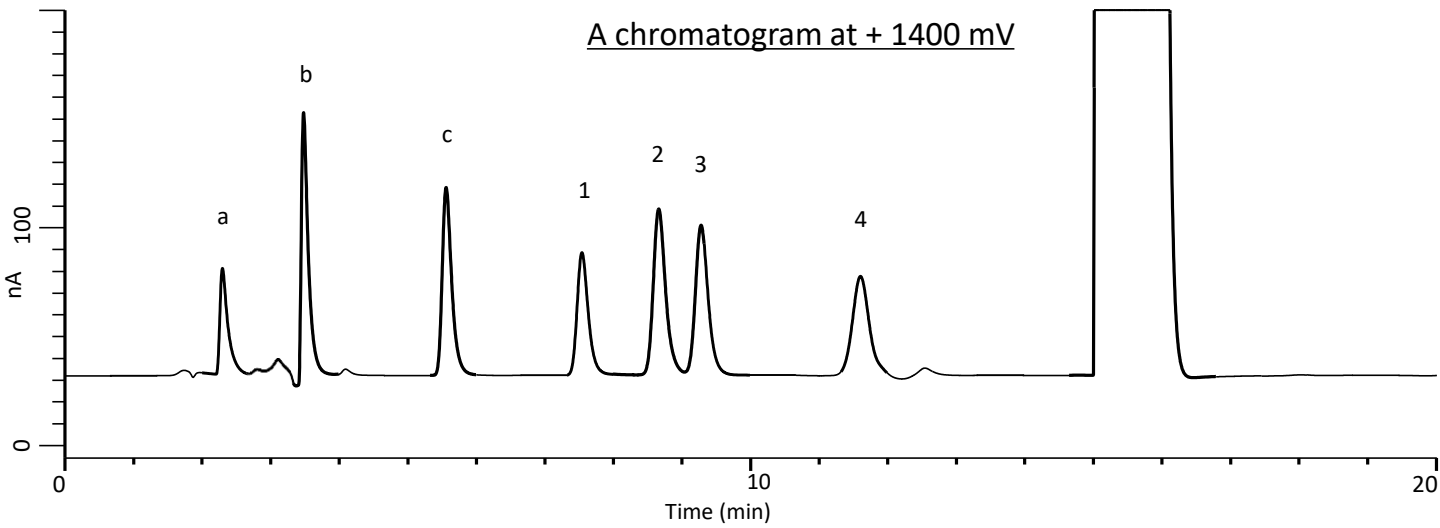

Pretreatment of urinary sample using MonoSpin PBA

MonoSpin is a series of spin columns for solid phase extraction (SPE). Owing to the high permeability of monolithic silica disk packed into the spin column, the procedures, such as conditioning, sample loading, washing, and elution can be carried out only by centrifuging the column. It is also the advantage that the elution volume is only 200 μL . Among the series of MonoSpin, MonoSpin PBA, which has phenylboronic acid as a functional group, can adsorb *cis*-hydroxyl group containing compounds selectively.

An Example of Procedures

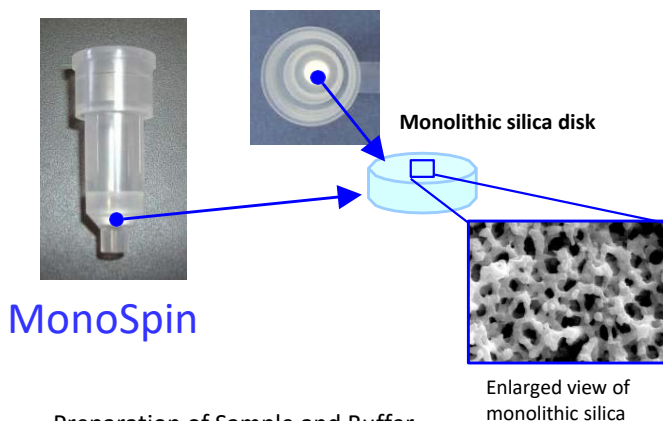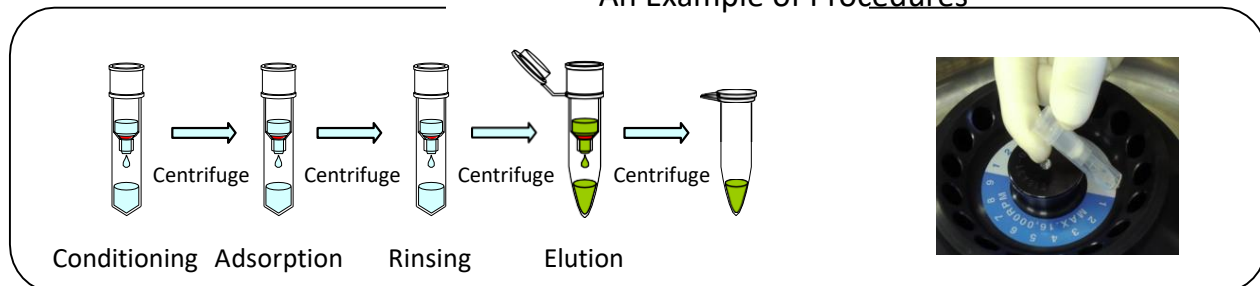

MonoSpin

Preparation of Sample and Buffer

Urine sample: Add DHBA solution as internal standard in advance. Buffer A: 1% acetic acid aqueous solution

Buffer B: 100 mM di-potassium hydrogen aqueous solution (The pH was adjusted to 8.0 by adding phosphoric acid)


Buffer C: 1 M di-potassium hydrogen aqueous solution (The pH was adjusted to 8.0 by adding phosphoric acid)

Procedures for purification of catecholamines

- Attach the spin column to tube for waste fluid
- ↓ + Buffer A 200 μL Centrifuge at 10,000 g for 1 min
- ↓ + Buffer B 200 μL Centrifuge at 10,000 g for 1 min
- ↓ + Urine sample 200 μL
- ↓ + Buffer C 50 μL Centrifuge at 10,000 g for 1 min
- ↓ + Buffer B 200 μL Centrifuge at 10,000 g for 1 min
- Put the spin column into collection tube
- ↓ + Buffer A 200 μL Centrifuge at 10,000 g for 1 min
- ↓
- Collected solution was injected into HPLC system


The series of MonoSpin

MonoSpin C18

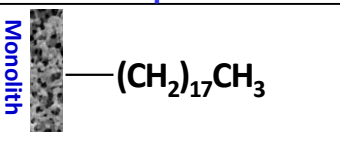


Octadecyl group is chemically bonded, and non-polar compounds can be retained because of its hydrophobic interaction. It can be used for extraction or desalting.

MonoSpin SAX

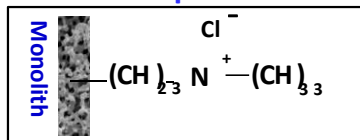


Trimethylaminopropyl group is bonded. It offers strong anion-exchange and weak hydrophobic interaction. It is suitable for extraction of acidic drugs.

MonoSpin NH₂

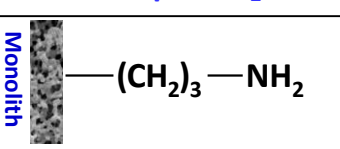


Aminopropyl group is bonded. It is suitable for extraction of hydrophilic compounds, such as sugar chain.

MonoSpin PBA

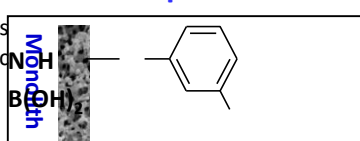


Phenylboronic acid is chemically bonded. Compounds containing *cis*-diol group can be retained with high selectivity.

MonoSpin SCX

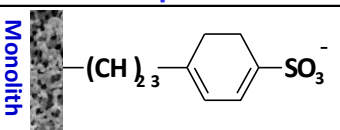

Propylbenzenesulfonic acid is bonded. It offers strong cation-exchange and hydrophobic interaction. It is suitable for extraction of basic drugs.

MonoSpin TiO₂

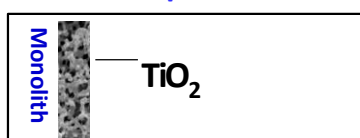


Monolithic silica is coated with titanium dioxide. It is suitable for extraction of phosphate-containing compounds.

(used in this note)


Without any pretreatment

Many interfering peaks were detected.

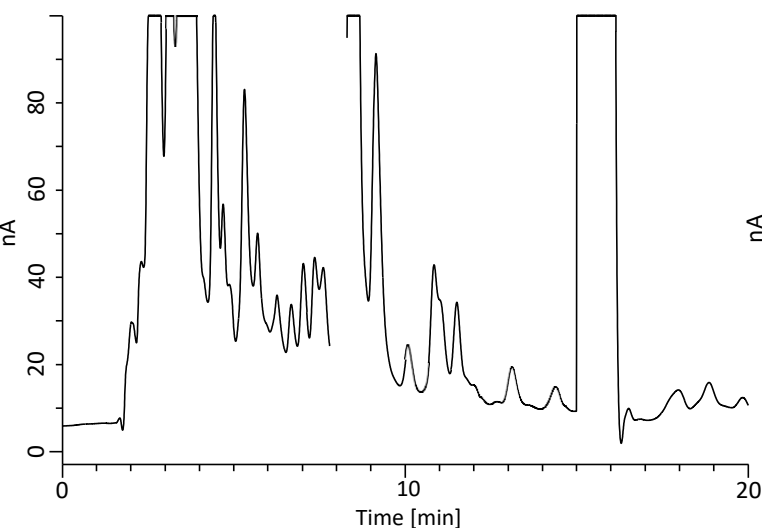


After pretreatment using MonoSpin PBA

Almost all interfering peaks were eliminated by the purification. The recovery ration of DHBA was 96.4 %.

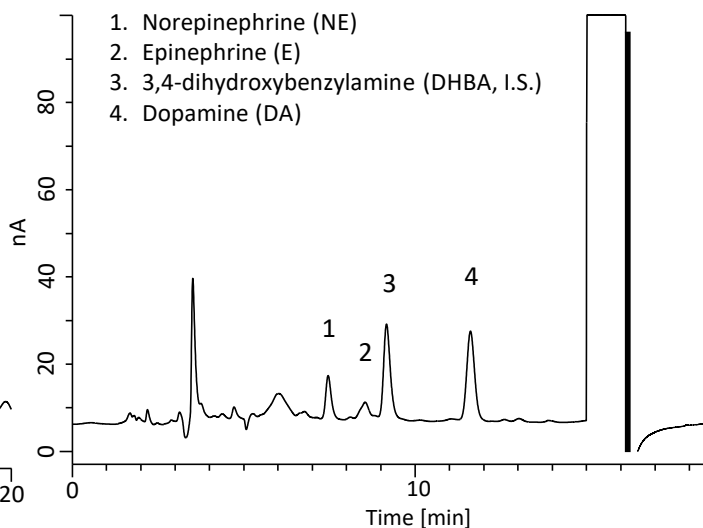

A standard addition plot

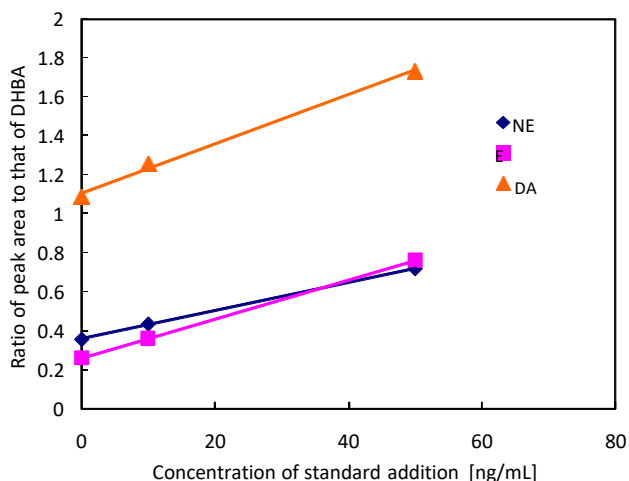

	Coefficient of variation	Obtained concentration of peak area (n=4)	[ng/mL]
NE	2.4 %	49.0	
E	6.9 %	25.9	
DA	0.8 %	85.5	

* We are grateful to Dr. Makoto Tsunoda (University of Tokyo) for his valuable suggestion and discussion.

GL Sciences disclaims any and all responsibility for any injury or damage which may be caused by this data directly or indirectly. We reserve the right to amend this information or data at any time and without any prior announcement.

GL Sciences, Inc. Japan

22-1 Nishishinjuku 6-Chome
Shinjuku-ku, Tokyo,
163-1130, Japan
Phone: +81-3-5323-6620
Fax: +81-3-5323-6621
Email: world@glsc.co.jp
Web: www.glsciences.com

GL Sciences B.V.

De Sleutel 9
5652 AS Eindhoven
The Netherlands
Phone: +31 (0)40 254 95 31
Email: info@glsciences.eu
Web: www.glsciences.eu

GL Sciences (ShangHai) Ltd.

Tower B, Room 2003,
Far East International Plaza,
NO,317 Xianxia Road,
Changning District.
Shanghai, China P.C. 200032
Phone: +86 (0)21-6278-2272
Email: contact@glsciences.com.cn
Web: www.glsciences.com.cn

GL Sciences, Inc. USA

4733 Torrance Blvd. Suite 255
Torrance, CA 90503
Phone: 310-265-4424
Fax: 310-265-4425
Email: info@glsciencesinc.com
Web: www.glsciencesinc.com

International Distributors

Visit our Website at:
<https://www.glsciences.com/company/distributor.html>

