


Analysis of Carbon dioxide

Specification

One GC Channel

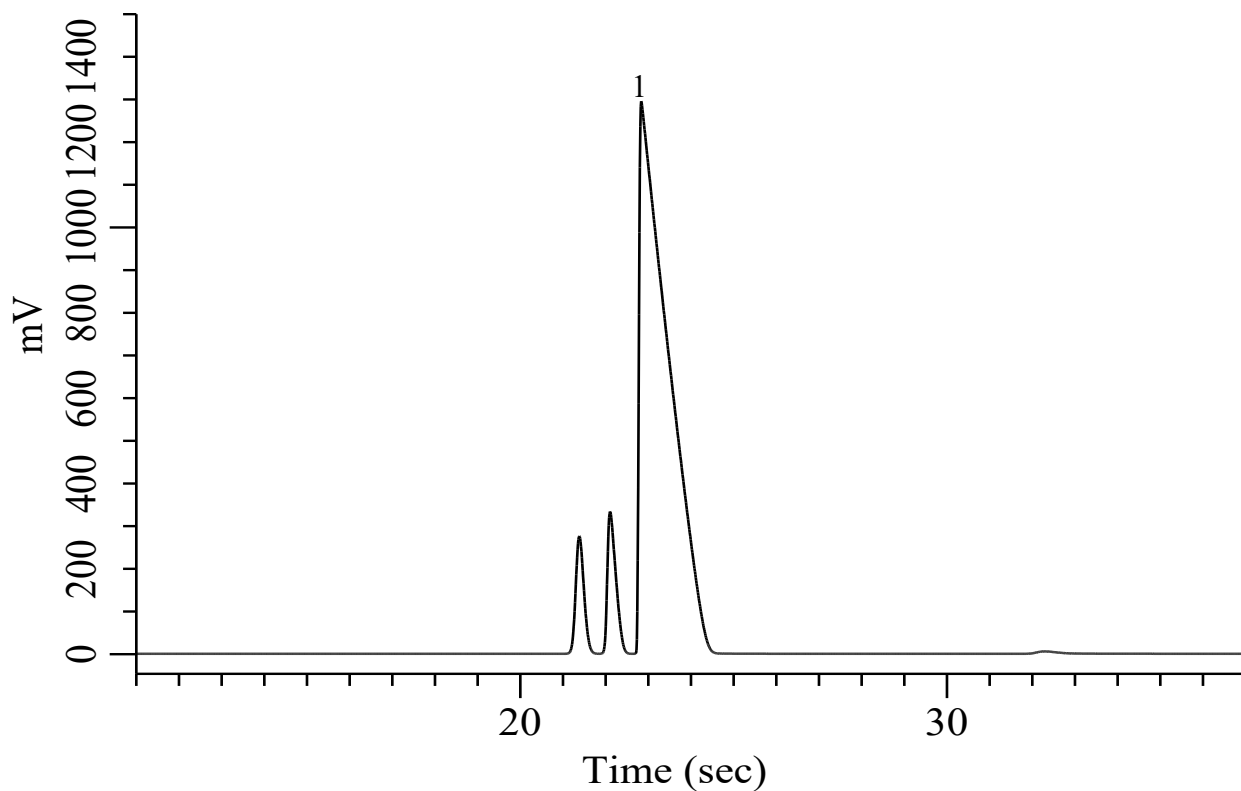

Conditions

System : Micro GC
Column : PoraPLOT Q 10 m
Column Temp. : 100 °C
Carrier Gas : He 190 kPa
Inject Time : 40 msec

Analyte:

1. Carbon dioxide (CO₂) 90 % (v/v)
 Balance Gas CH₄