


Analysis of Carbon dioxide, Ammonia

Specification

One GC Channel

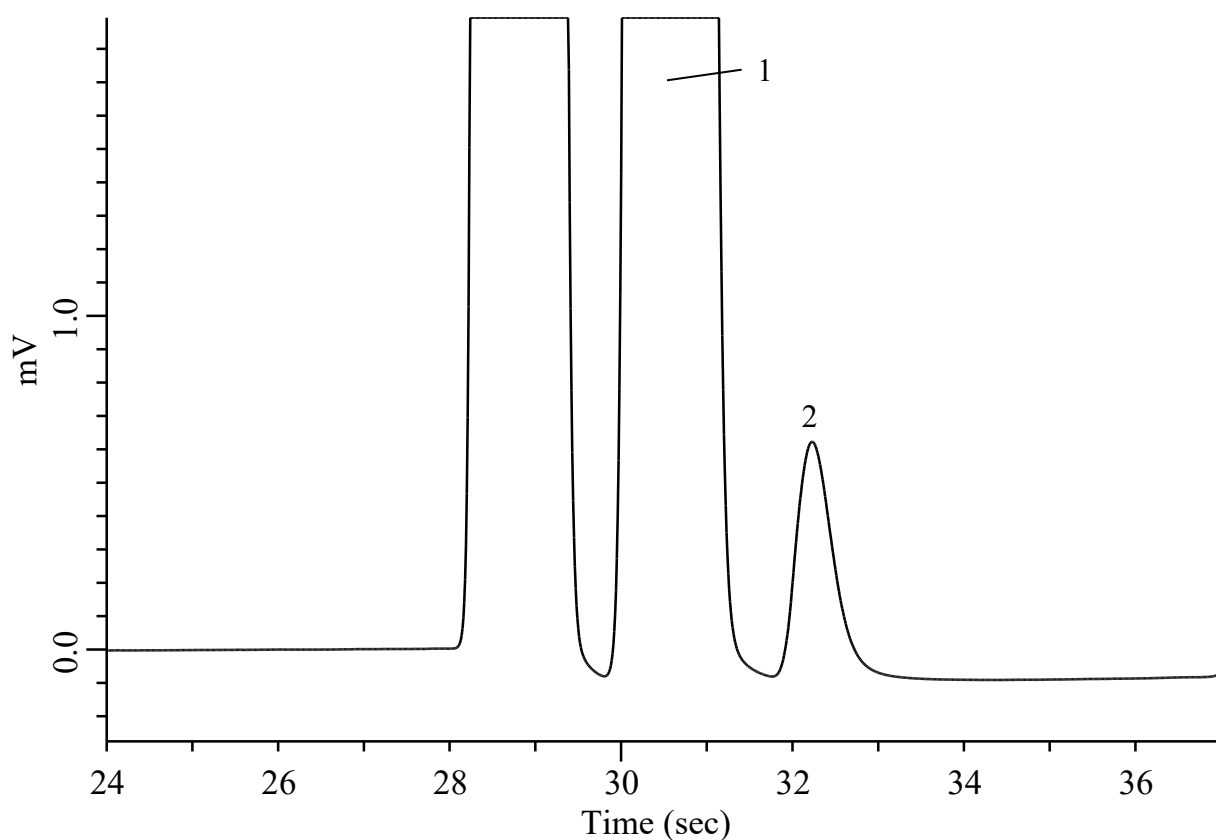

Conditions

System : Micro GC
Column : CP-Volamine 15 m
Column Temp. : 40 °C
Carrier Gas : He 190 kPa
Inject Time : 40 msec

Analyte:

1. Carbon dioxide 10 % (v/v)
 2. Ammonia 500 ppm (v/v)

Balance Gas N₂